

# Temperature Log

The Jikei University Hospital

Location : Pharmaceutical department

Refrigerator Name: ER-49C

Acceptable Temperature Range : 2°C to 8°C

Temperature Logger/ID : RTR501BL/ 52802EFD (Calibration date ; 29 Sep 2025)


※The certification period is one year from the date of calibration.

\*error  
02/Feb/2026  
S-H

Month/Year (年月) (MMM/YYYY) : <u>Jan/2025</u>	Confirmation Time 確認時間	Alarm: No or Yes アラームの有無	Initials (確認者)
Date(日)			
1	:	No · Yes	
2	:	No · Yes	
3	:	No · Yes	
4	:	No · Yes	
5	10 : 30	<input checked="" type="radio"/> No · Yes	S-H
6	8 : 30	<input checked="" type="radio"/> No · Yes	S-H
7	8 : 30	<input checked="" type="radio"/> No · Yes	S-H
8	8 : 30	<input checked="" type="radio"/> No · Yes	S-H
9	9 : 30	<input checked="" type="radio"/> No · Yes	S-H
10	8 : 30	<input checked="" type="radio"/> No · Yes	S-H
11	:	No · Yes	
12	:	No · Yes	
13	9 : 20	<input checked="" type="radio"/> No · Yes	R-Y
14	8 : 30	<input checked="" type="radio"/> No · Yes	S-H
15	8 : 30	<input checked="" type="radio"/> No · Yes	S-H
16	9 : 00	<input checked="" type="radio"/> No · Yes	S-H
17	9 : 00	<input checked="" type="radio"/> No · Yes	R-Y
18	:	No · Yes	
19	10 : 30	<input checked="" type="radio"/> No · Yes	R-Y
20	8 : 50	<input checked="" type="radio"/> No · Yes	Y.N
21	8 : 30	<input checked="" type="radio"/> No · Yes	S-H
22	8 : 30	<input checked="" type="radio"/> No · Yes	S-H
23	12 : 00	<input checked="" type="radio"/> No · Yes	R-Y
24	8 : 30	<input checked="" type="radio"/> No · Yes	Y.N
25	:	No · Yes	
26	8 : 30	<input checked="" type="radio"/> No · Yes	S-H
27	17 : 00	<input checked="" type="radio"/> No · Yes	S-H
28	9 : 00	<input checked="" type="radio"/> No · Yes	S-H
29	8 : 30	<input checked="" type="radio"/> No · Yes	Y.N
30	16 : 30	<input checked="" type="radio"/> No · Yes	S-H
31	8 : 30	<input checked="" type="radio"/> No · Yes	S-H

Investigational Product Manager's Signature: Shunsuke Hitosuzuki

Date: 02 Feb 2026

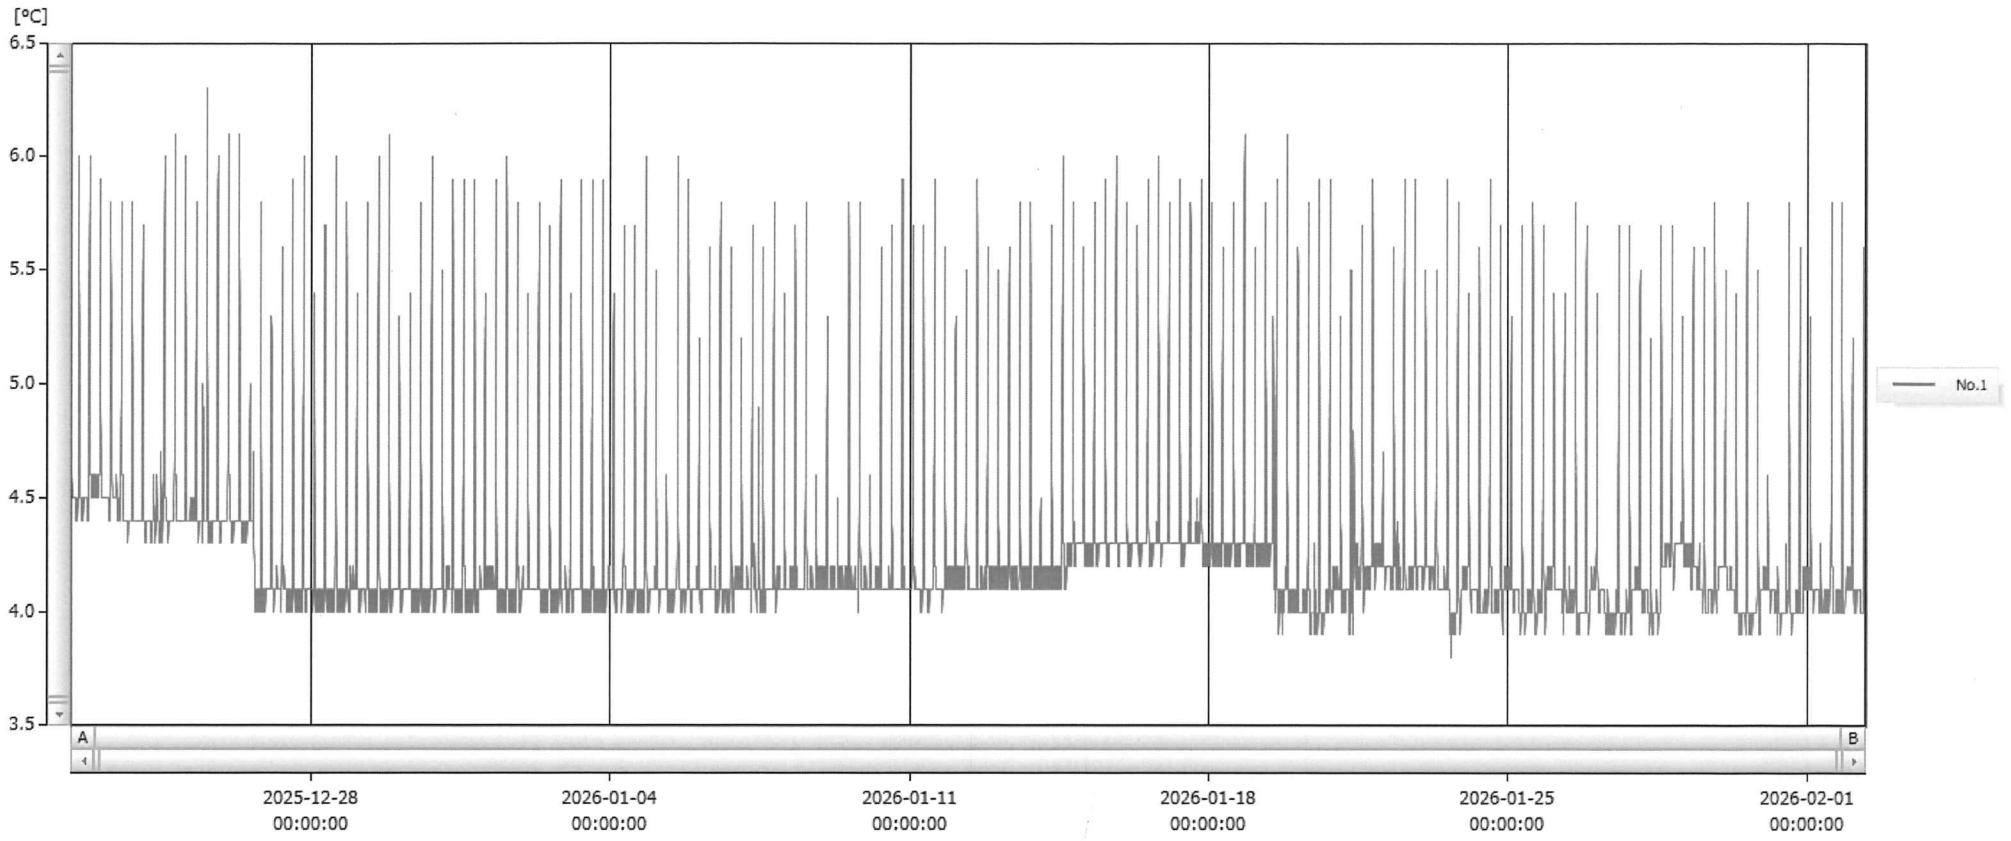

表示範囲 2025-12-22 09:01:00 - 2026-02-02 08:57:00  
 計算範囲 2025-12-22 09:01:00 - 2026-02-02 08:57:00

*Shunsuke Hitosuz* 02/Feb/2026

No.	チャンネル名	記録間隔	データ数	単位	最大値	最小値	平均値
No.1	冷所A	5 min.	12096	°C	6.3	3.8	4.2