

# Temperature Log

The Jikei University Hospital

Location : Pharmaceutical department

Refrigerator Name: ER-49C

Acceptable Temperature Range : 2°C to 8°C

Temperature Logger/ID : RTR501BL/ 52802EFD (Calibration date ; 29 Sep 2025)


※The certification period is one year from the date of calibration.

Month/Year (年月) (MMM/YYYY) : <u>Mar/2026</u>	Confirmation Time 確認時間	Alarm: No or Yes アラームの有無	Initials (確認者)
Date(日)			
1	:	<del>No · Yes</del>	
2	10 : 30	(No) · Yes	Y, N
3	14 : 30	(No) · Yes	S-H
4	8 : 30	(No) · Yes	S-H
5	9 : 20	(No) · Yes	S-H
6	9 : 30	(No) · Yes	R-Y
7	8 : 30	*1 (No) · Yes	S-H
8	:	<del>No · Yes</del>	
9	8 : 30	(No) · Yes	S-H
10	9 : 30	(No) · Yes	S-H
11	9 : 30	(No) · Yes	S-H
12	8 : 40	(No) · Yes	Y, N
13	8 : 30	(No) · Yes	S-H
14	9 : 30	(No) · Yes	S-H
15	:	<del>No · Yes</del>	
16	9 : 00	(No) · Yes	S-H
17	9 : 30	(No) · Yes	S-H
18	9 : 00	(No) · Yes	S-H
19	9 : 30	(No) · Yes	S-H
20	:	<del>No · Yes</del>	
21	11 : 20	(No) · Yes	Y, N
22	:	<del>No · Yes</del>	
23	8 : 30	(No) · Yes	Y, N
24	8 : 30	(No) · Yes	S-H
25	9 : 50	(No) · Yes	R-Y
26	9 : 15	(No) · Yes	S-H
27	11 : 00	(No) · Yes	S-H
28	8 : 30	(No) · Yes	Y, N
29	:	<del>No · Yes</del>	
30	10 : 30	(No) · Yes	S-H
31	14 : 00	(No) · Yes	S-H

\*error  
05 Mar 2026  
S-H

Investigational Product Manager's Signature: Shunsuke Hitosugi

Date: 06 Apr 2026

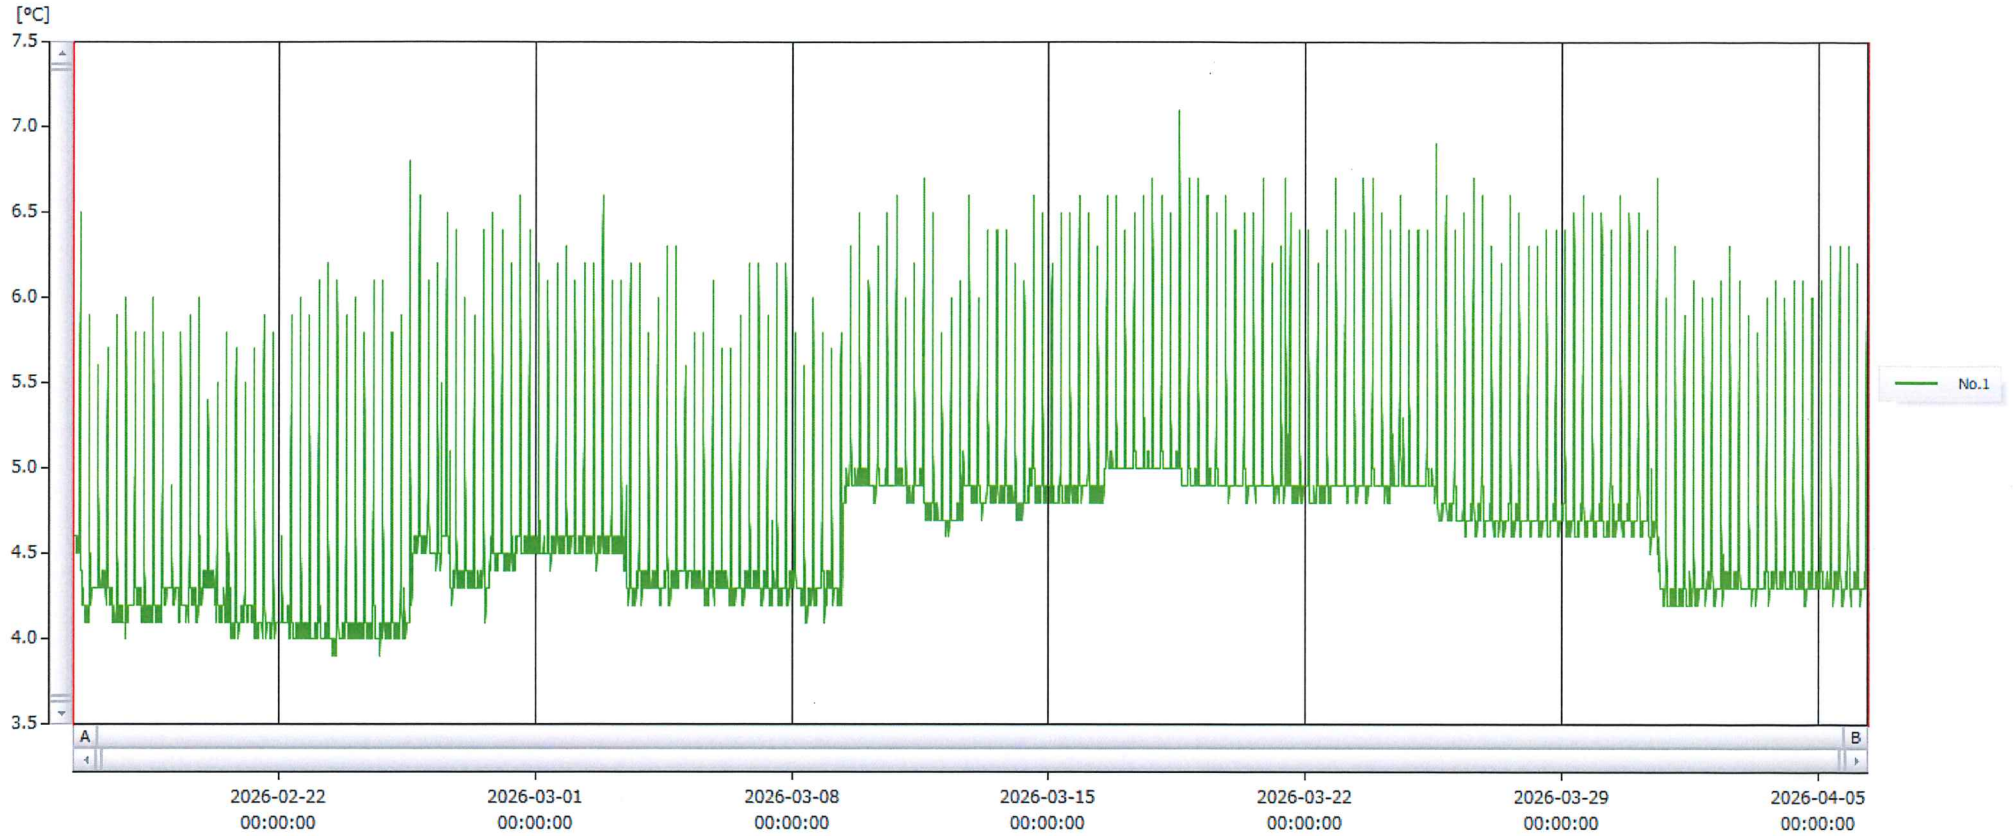

表示範囲 2026-02-16 09:02:00 - 2026-04-06 08:58:00

計算範囲 2026-02-16 09:02:00 - 2026-04-06 08:58:00

No.	チャンネル名	記録間隔	データ数	単位	最大値	最小値	平均値
No.1	冷所A	5 min.	14112	°C	7.1	3.9	4.7