

Temperature Log

The Jikei University Hospital
 Refrigerator Name: MPR-514-PJ
 Temperature Logger/ID : RTR501BL/ 52802EFE (Calibration date ; 29 Sep 2025)

Location : Pharmaceutical department
 Acceptable Temperature Range : 2°C to 8°C


※The certification period is one year from the date of calibration.

Month/Year (年月) (MMM/YYYY) : <i>Apr/2026</i>	Confirmation Time 確認時間	Alarm: No or Yes アラームの有無	Initials (確認者)
Date(日)			
1	11 : 00	<input checked="" type="radio"/> No · Yes	<i>P.Y</i>
2	8 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
3	8 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
4	16 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
5	:	No · Yes	
6	10 : 00	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
7	8 : 30	<input checked="" type="radio"/> No · Yes	<i>P.Y</i>
8	9 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
9	9 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
10	10 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
11	8 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
12	:	No · Yes	
13	8 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
14	8 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
15	9 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
16	8 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
17	9 : 00	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
18	9 : 10	<input checked="" type="radio"/> No · Yes	<i>P.Y</i>
19	:	No · Yes	
20	8 : 45	<input checked="" type="radio"/> No · Yes	<i>P.Y</i>
21	10 : 45	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
22	8 : 30	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
23	9 : 50	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
24	10 : 15	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
25	9 : 15	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
26	:	No · Yes	
27	9 : 00	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
28	15 : 00	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
29	:	No · Yes	
30	9 : 00	<input checked="" type="radio"/> No · Yes	<i>S.H</i>
31	:	No · Yes	

Investigational Product Manager's Signature: *Shimizu Hitosugi*

Date: *07 May 2026*

Shimsuke Hitosugi 07 May 2026

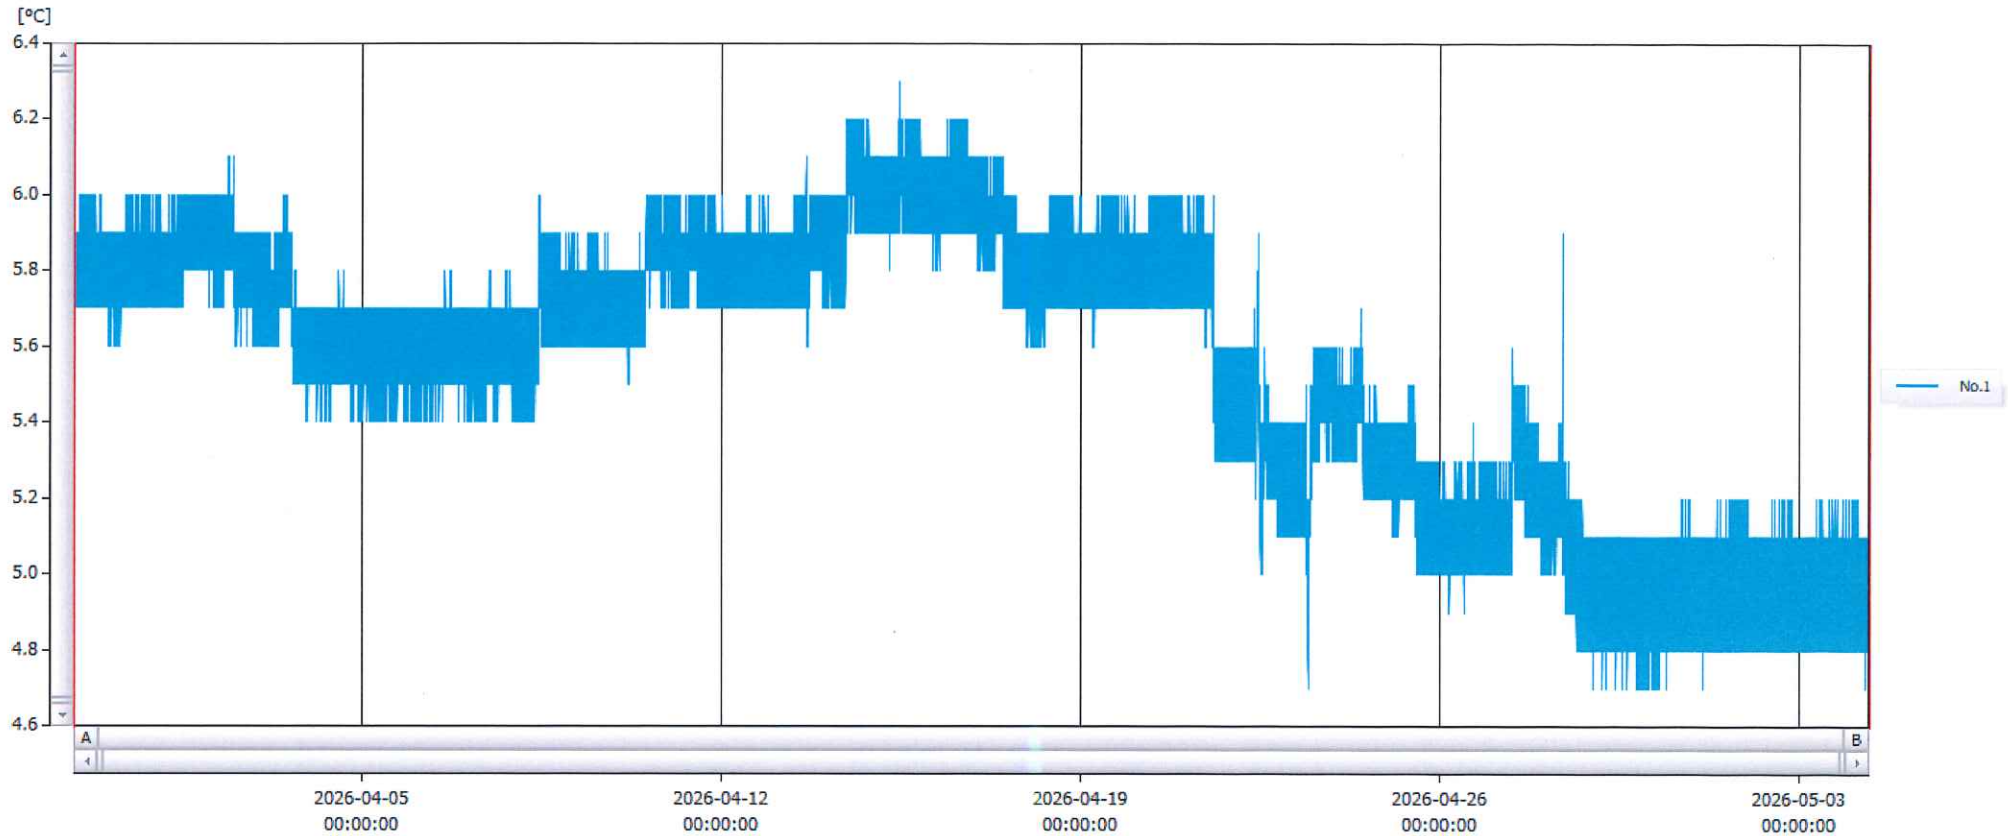

表示範囲 2026-03-30 09:03:00 - 2026-05-04 08:59:00

計算範囲 2026-03-30 09:03:00 - 2026-05-04 08:59:00

No.	チャンネル名	記録間隔	データ数	単位	最大値	最小値	平均値
No.1	冷所B	5 min.	10080	°C	6.3	4.7	5.6