Temperature Log

The Jikei University Hospital　　Location : Pharmaceutical department
Refrigerator Name:ER-49C　　Acceptable Temperature Range : 2℃ to 8℃
Temperature Logger/ID : RTR501BL/ 52802EFD (Calibration date ; 29 Sep 2025)
※The certification period is one year from the date of calibration.
★ Starting September 28, 2026, management will be handled by the new logger. RTR501BL/52801114 (Calibration date ; 18 Aug 2026)


Month/Year (年月) (MMM/YYYY) : Sep/2026 Date(日)	Confirmation Time 確認時間	Alarm: No or Yes アラームの有無	Initials (確認者)
1	15 : 00	(No) · Yes	S-H
2	10 : 15	(No) · Yes	R.Y
3	10 : 00	(No) · Yes	S-H
4	9 : 00	(No) · Yes	S-H
5	9 : 00	(No) · Yes	S-H
6	:	~~No · Yes~~	
7	11 : 00	(No) · Yes	Y, N
8	9 : 00	(No) · Yes	S-H
9	9 : 00	(No) · Yes	S-H
10	14 : 00	(No) · Yes	S-H
11	9 : 00	(No) · Yes	S-H
12	9 : 00	(No) · Yes	S-H
13	:	~~No · Yes~~	
14	9 : 30	(No) · Yes	S-H
15	10 : 05	(No) · Yes	R.Y
16	11 : 30	(No) · Yes	S-H
17	12 : 00	(No) · Yes	S-H
18	9 : 00	(No) · Yes	S-H
19	9 : 30	(No) · Yes	S-H
20	:	No · Yes	
21	:	No · ~~Yes~~	
22	:	No · Yes	
23	:	No · Yes	
24	9 : 00	(No) · Yes	S-H
25	13 : 00	(No) · Yes	S-H
26	9 : 00	(No) · Yes	S-H
27	:	~~No · Yes~~	
28	9 : 00	(No) · Yes	S-H
29	9 : 30	(No) · Yes	S-H
30	10 : 30	(No) · Yes	Y, N
31	:	~~No · Yes~~	

Investigational Product Manager's Signature: Shunsuke Hitosugi　　Date: 05 Oct 2026

T&D Graph

2026-10-05 12:03:59

Shunsuke Hitosugi; 06 Oct 2026

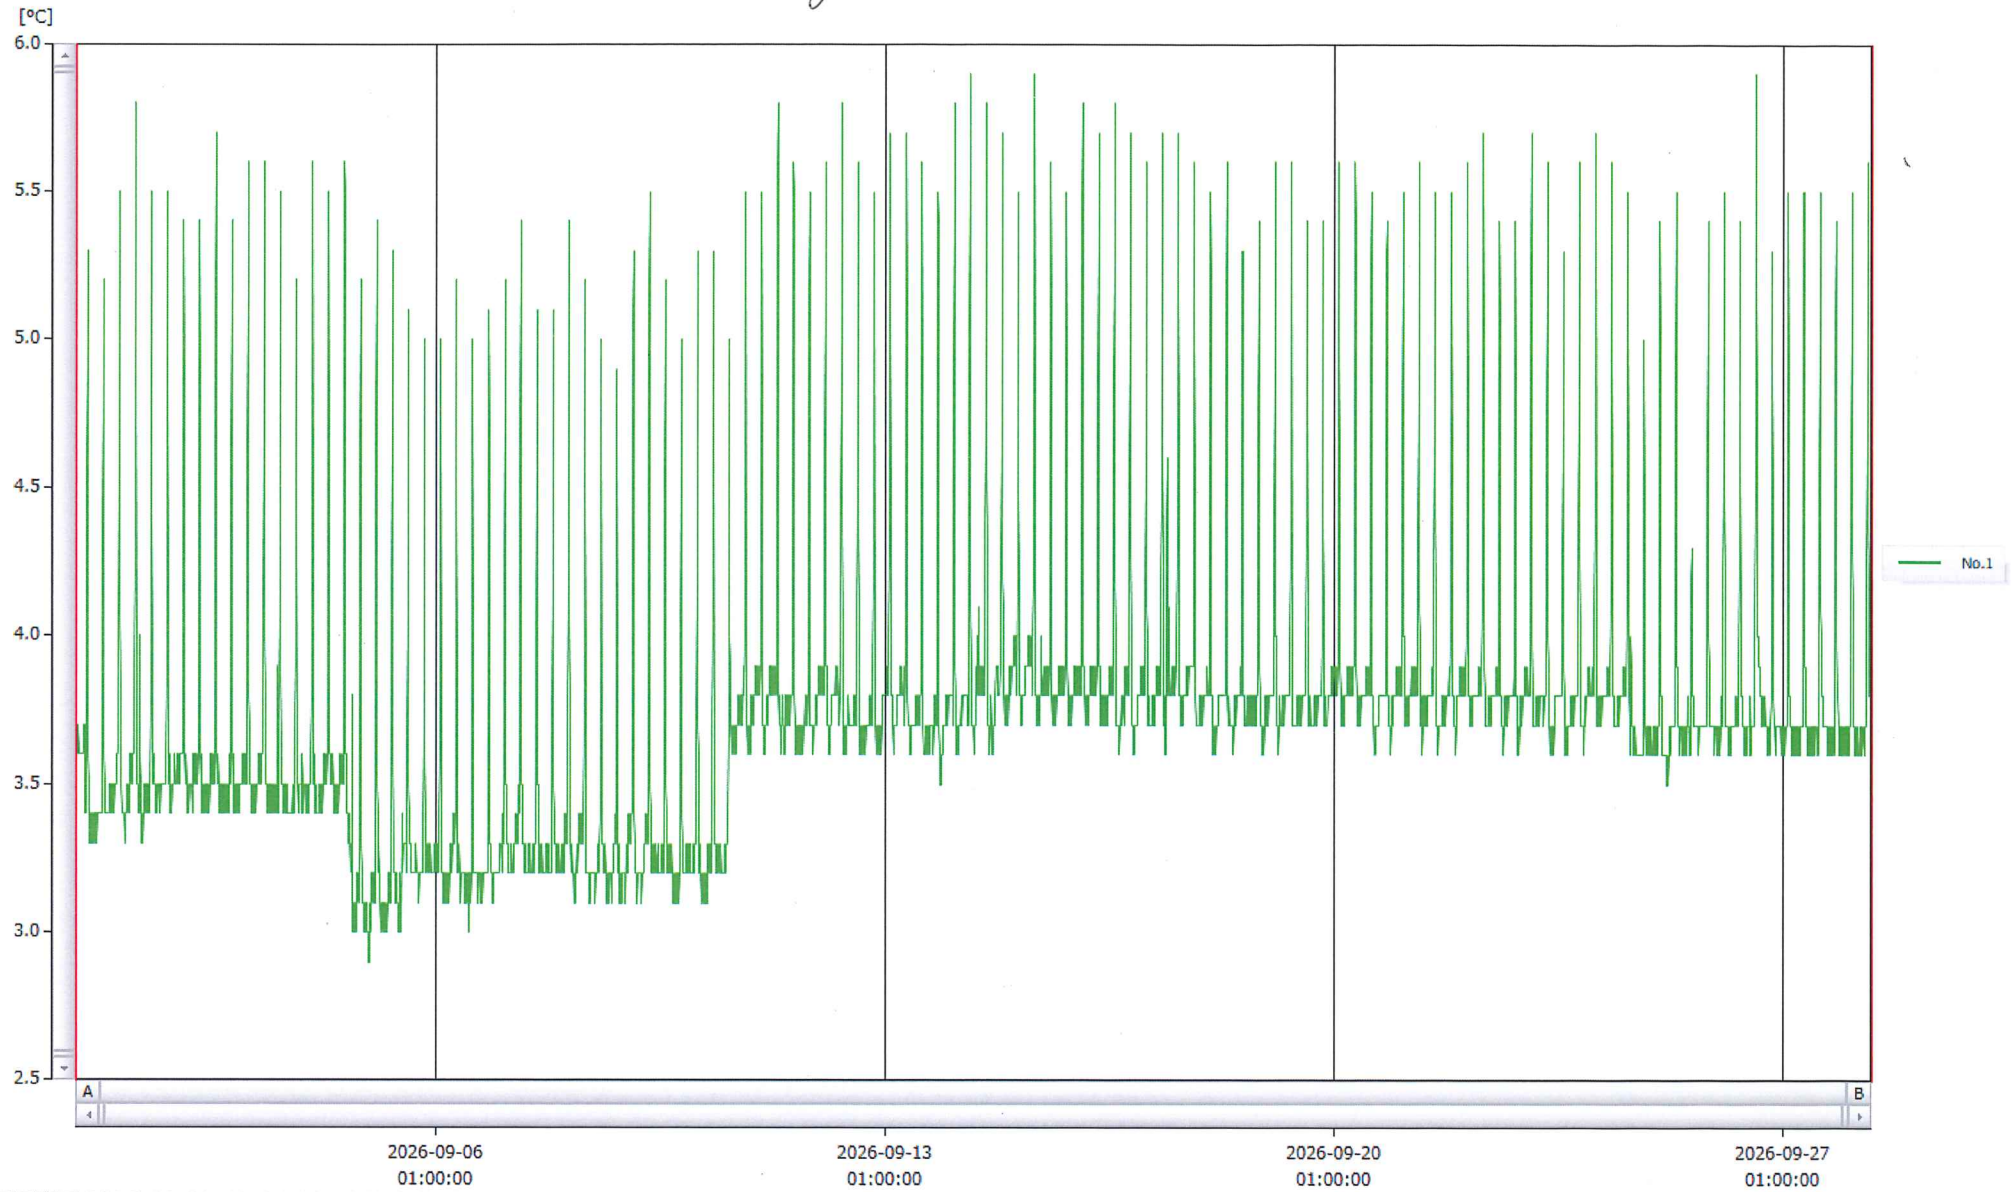

表示範囲 2026-08-31 10:01:00 - 2026-09-28 09:57:00
計算範囲 2026-08-31 10:01:00 - 2026-09-28 09:57:00


No.	チャンネル名	記録間隔	データ数	単位	最大値	最小値	平均値
No.1	冷所A	5 min.	8064	°C	5.9	2.9	3.7

S/N : 52802 EFD

T&D Graph

2026-10-05 12:05:58

Shunsuke Hitosugi 06 Oct 2026

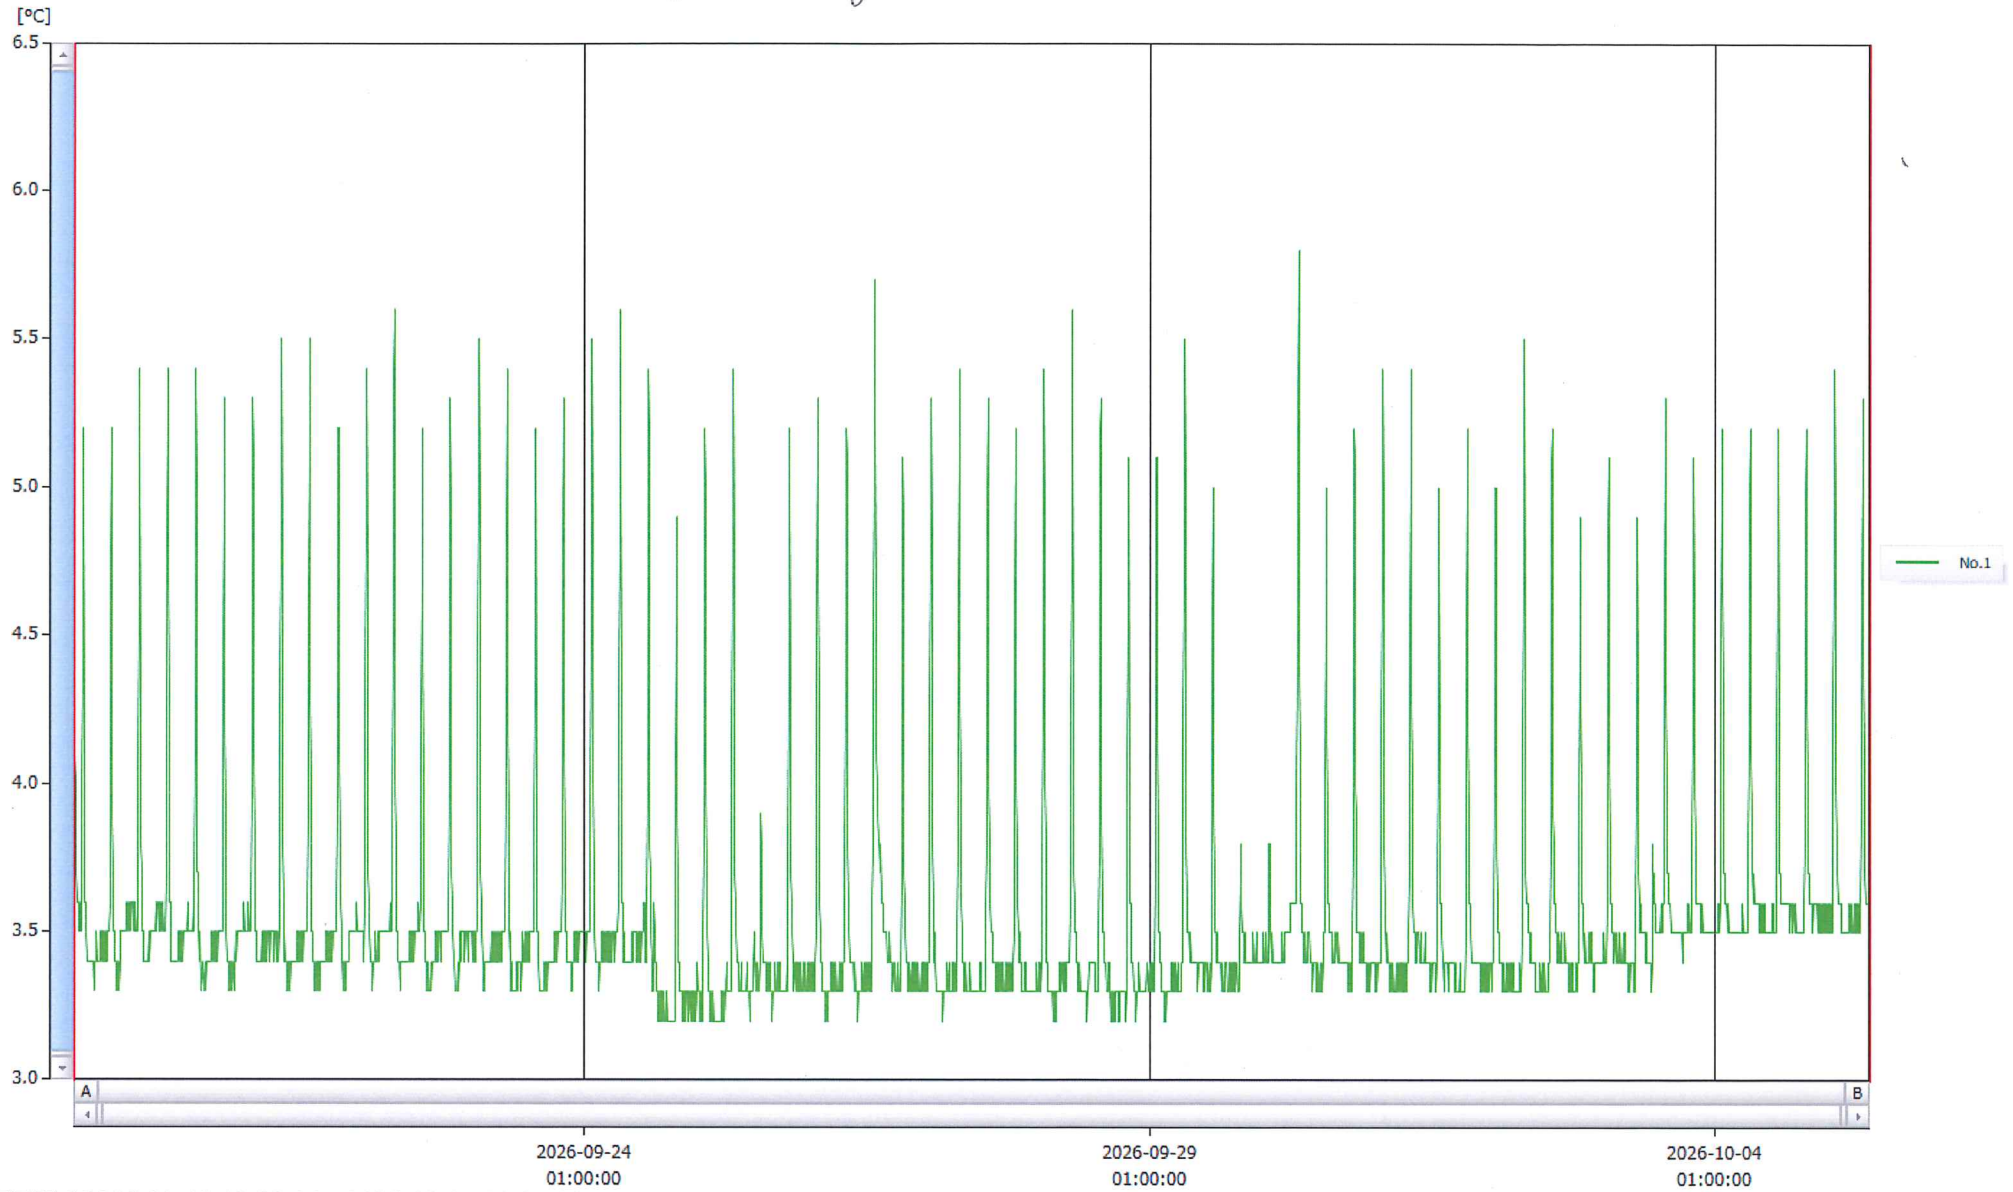

表示範囲 2026-09-19 12:29:00 - 2026-10-05 10:01:00
計算範囲 2026-09-19 12:29:00 - 2026-10-05 10:01:00

No.	チャンネル名	記録間隔	データ数	単位	最大値	最小値	平均値
No.1	冷A2609	5 min.	4579	°C	6.0	3.2	3.5

↳ S/N : 52805114